

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDUHS3-0080

Certification Date:

3.4.21

Technician:

am

Re-Certification Due Date:

3.4.22

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-022

Certification Date:

3.4.21

Next Certification Due:


3.4.22

Probe Value:

106

Dräger, Inc.

am

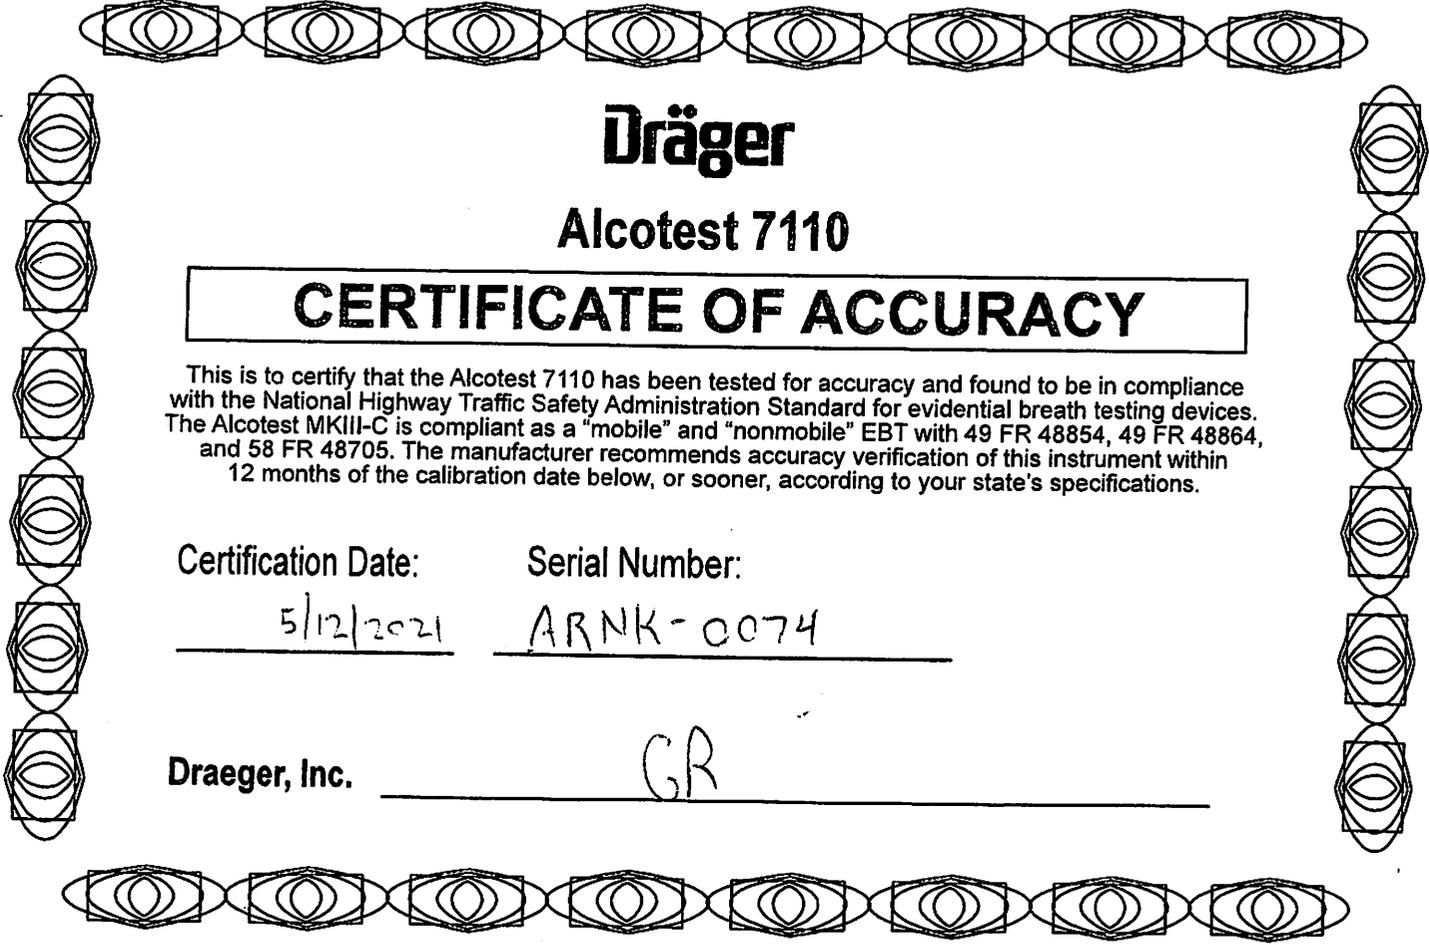

Dräger

Alcotest 7110

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

5/12/2021

ARNK-0074

Draeger, Inc. GR

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Matthew R. Watson
New Jersey State Police



IS QUALIFIED AND COMPETENT TO CONDUCT CERTIFICATE COURSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1984 IN THE OPERATION OF THE **7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 10th DAY OF August

TWO THOUSAND AND 100

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-8-12	GCPA	Wm Long
2. 7/14/15	CMPA	Adama Sanders
3. 3/23/17	Lakehurst	Michelle Jordan
4. 4-20-19	GCPA	Wm Long
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2938 (Rev. 03/10)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Matthew R. Watson
Breath Test Coordinator/Instructor



IS QUALIFIED AND COMPETENT TO CONDUCT CERTIFICATE COURSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1984 IN THE OPERATION OF THE **7110 MKIII-C**
A METHOD TO DETERMINE INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 16th DAY OF June

TWO THOUSAND AND Sixteen

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2938 (Rev. 08/13)



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger, Inc.

ANALYSIS DATE: 01/28/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21010


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 13, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29 day of January, 2021.


Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 6/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Handwritten mark or signature at the top left.

Handwritten text or header at the top of the page.

Printed text or header in the upper right quadrant.

First paragraph of the main body text.

Second paragraph of the main body text.

Third paragraph of the main body text.

Section header or sub-header in the middle of the page.

Text block on the left side of the middle section.

Text block on the right side of the middle section.

Text block at the bottom of the middle section.

Section header or title at the bottom of the page.

Text block in the bottom left corner.

Text block in the bottom center of the page.

Text block in the bottom right corner.



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/17/2020

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 20280

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1949 to 0.1977 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 17, 2022.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of July, 2020.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/07/2020

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 20270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0968 to 0.0974 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 11, 2022.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of August, 2020.

Notary Public



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/29/2020

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 20260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0481 to 0.0486 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 08, 2022.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of August, 2020.
Marilynne Kuecker
Notary



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor
SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General
PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/25/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19280

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 16, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of October, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11236881

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 20 Apr 2020

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11236881

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by : VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601, S/N: 200247685 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Probe	128	06 Jun 2020	15-C2Z0T-40-1
Thermistor Module	A17118	21 May 2020	1000441638
Thermistor Module	A27129	04 Feb 2021	1000451212
Temperature Calibration Bath	A73332		
Temperature Probe	3039	06 Jun 2020	15-C2Z0T-20-1
Temperature Calibration Bath	A79341		
Temperature Calibration Bath	B16388		
Temperature Probe	5267	21 Feb 2021	C0220028
Temperature Calibration Bath	B93537		
Thermistor Module	B96382	19 Aug 2020	B9628006
Temperature Probe	5407	19 Aug 2020	B9801028

Certificate Information:

Technician: 420 Procedure: CAL-06 Cal Date: 20 Apr 2020 Cal Due Date: 20 Apr 2022
 Test Conditions: 59.19%RH 23.31°C 1014mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.004	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.001	25.004	Y	24.951	25.051	0.0087	>4:1
°C	N.A.	N.A.		50.000	50.004	Y	49.95	50.05	0.0087	>4:1
°C	N.A.	N.A.		100.004	100.006	Y	99.954	100.054	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement": (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Marisa Elms
Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
 Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-D1805-2006-AQ-HOU-ANAB.
 International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:

DDXNS3-D153

Certification Date:

3.22.21

Technician:

MB

Re-Certification Due Date:

3.22.22

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDLBP3-0075

Certification Date:

3.24.21

Next Certification Due:

3.24.22

Probe Value:

102

Draeger, Inc.

MB



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:
DDRFS3-0009

Certification Date:
3.17.21

Technician:
[Signature]

Re-Certification Due Date:
3.17.22



Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: _____

Serial Number:
DDWFS3-0225

Certification Date:
3.24.21

Technician:
[Signature]

Re-Certification Due Date:
3.24.22



**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Tpr. I Matthew R. Watson
Name

7078
Badge No.

Location:

South Brunswick Police
Agency

ARNK-0074
Alcotest Serial No.

Equipment:

200247685
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDRF53-0009	08:13D	09:15D	34.0°C
0.08%	DDWF53-0225	08:13D	09:16D	34.0°C
0.10%	DDUH 53-0080	08:13D	09:17D	34.0°C
0.16%	DDXN 53-0153	08:13D	09:19D	33.9°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr. I Matthew R. Watson #7078
Coordinator's Signature

06/16/2021
Date

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARNK-0074
Location:	SOUTH BRUNSWICK POLICE		
Calibration File No.:	01162	Calib. Date:	06/16/2021
Certification File No.:	01163	Cert. No.:	00047
Linearity File No.:	01164	Cert. Date:	06/16/2021
Solution File No.:	01165	Lin. No.:	00034
Sequential File No.:	01165	Lin. Date:	06/16/2021
		Soln. No.:	00253
		Soln. Date:	06/16/2021
		File Date:	06/16/2021
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUH S3-0080
Solution Control Lot:	21010	Expires:	01/13/2023
		Bottle No.:	1193

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:54D		
Control 1 EC	0.101%	10:55D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	10:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:55D		
Control 2 EC	0.100%	10:56D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	10:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:56D		
Control 3 EC	0.100%	10:57D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	10:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:58D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDEEP2-022 (MRW)

Changed By:

Last Name: WATSON	First Name: MATTHEW	MI: R
Signature: <u></u>	Badge No.: 7078	Date: 06/16/2021

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0074
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 01162 Calib. Date: 06/16/2021 Calib. No.: 00047
Certification File No.: 01163 Cert. Date: 06/16/2021 Cert. No.: 00034
Linearity File No.: 01164 Lin. Date: 06/16/2021 Lin. No.: 00034
Solution File No.: 01160 Soln. Date: 05/12/2021 Soln. No.: 00252
Sequential File No.: 01164 File Date: 06/16/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRF S3-0009
Control Solution %: 0.040% Expires: 06/08/2022
Solution Control Lot: 20260 Bottle No.: 0823

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWF S3-0225
Control Solution %: 0.080% Expires: 06/11/2022
Solution Control Lot: 20270 Bottle No.: 0506

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXN S3-0153
Control Solution %: 0.160% Expires: 06/17/2022
Solution Control Lot: 20280 Bottle No.: 1190

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:37D		
Control 1 EC	0.041%	09:38D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.041%	09:38D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:39D		
Control 2 EC	0.040%	09:40D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.041%	09:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:41D		
Control 3 EC	0.080%	09:42D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43D		
Control 4 EC	0.080%	09:44D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45D		
Control 5 EC	0.158%	09:46D	33.8°C	*** TEST PASSED ***
Control 5 IR	0.158%	09:46D	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47D		
Control 6 EC	0.158%	09:48D	33.8°C	*** TEST PASSED ***
Control 6 IR	0.158%	09:48D	33.8°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49D		

All tests within acceptable tolerance.

Coordinator

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature: Tpc. I Matthew A. Watson #7078

Badge No.: 7078

Date: 06/16/2021

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARNK-0074
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 01162 Calib. Date: 06/16/2021 Calib. No.: 00047
Certification File No.: 01163 Cert. Date: 06/16/2021 Cert. No.: 00034
Linearity File No.: 01145 Lin. Date: 12/31/2020 Lin. No.: 00033
Solution File No.: 01160 Soln. Date: 05/12/2021 Soln. No.: 00252
Sequential File No.: 01163 File Date: 06/16/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0080
Control Solution %: 0.100% Expires: 10/16/2021
Solution Control Lot: 19280 Bottle No.: 0457

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:24D		
Control 1 EC	0.099%	09:25D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:25D		
Control 2 EC	0.099%	09:26D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:26D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:26D		
Control 3 EC	0.099%	09:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:28D		

All tests within acceptable tolerance.

Coordinator

Last Name: WATSON

First Name: MATTHEW

MI: R

Signature: Tpr. J. Watson # 7078

Badge No.: 7078

Date: 06/16/2021

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Record

Equipment

Alcotest 7110 MKIII-C
SOUTH BRUNSWICK POLICE
Serial No.: ARNK-0074

Calibration File No.:	01162	Calib. Date:	06/16/2021	Calib. No.:	00047
Certification File No.:	01144	Cert. Date:	12/31/2020	Cert. No.:	00033
Linearity File No.:	01145	Lin. Date:	12/31/2020	Lin. No.:	00033
Solution File No.:	01160	Soln. Date:	05/12/2021	Soln. No.:	00252
Sequential File No.:	01162	File Date:	06/16/2021		

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 19280

Model No.: CU-34
Serial No.: DDUH S3-0080
Expires: 10/16/2021
Bottle No.: 0457


Coordinator

Last Name: WATSON
First Name: MATTHEW
MI: R

Signature: *Tric. I. Watson* #2078
Badge No.: 7078
Date: 06/16/2021

*Black Key Temperature Probe Serial.....# DDLSP3-0075 MRW

*Digital NIST Temperature Measuring System Serial.....# 200247685 MRW

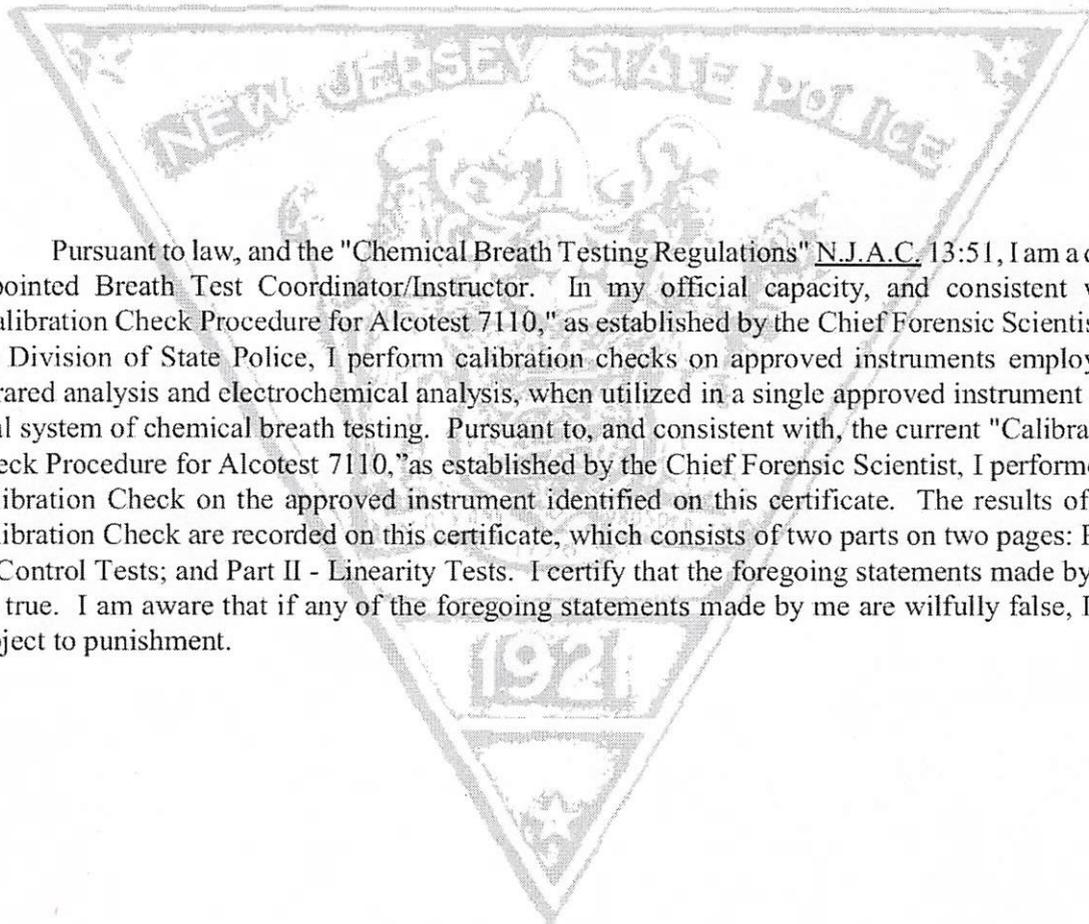

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.