

## ALCOTEST 9510 PARAMETER REPORT

### Equipment

Serial No.: ARMJ-0294  
Firmware: 8326739 1.5  
WinCE application: 8326738 2.9  
Configuration: 8326737 3.10

Date: 01/15/2026  
Time: 06:47:25

### Parameter

min. blow time	5.0	s
min. breath volume for females of age 60+	1.2	L
min. breath volume for all other	1.5	L
min. blow flow	4.5	L/min
plateau detection limit	4	%
plateau detection start conc.	70	microgram/L
neg. flow detection (part. vacuum)	10.0	hPa
neg. flow detection sensitivity	10	
cal. gas abort volume	0.4	L
result-to-zero limit	0.0050	%BAC
ambient air check limit	0.0049	%BAC
interference det. d-criterion limit abs.	38	microgram/L
interference det. d-criterion limit rel.	10.0	%
interference det. t-criterion limit abs.	8	microgram/L
interference det. t-criterion limit rel.	2.1	%
IR CO2 offset	10	microgram/L
IR H2O offset	4	microgram/L
EC H2O offset	0	microgram/L
Value-based EC aging comp. on/off (1/0)	0	
Time-based EC aging comp. on/off (1/0)	1	
Time-based EC aging comp. per month	0.2	%
Time-based EC aging comp. maximum	3.0	%
EC fatigue comp. max. sum	15000	
EC fatigue comp. factor	50	
EC fatigue comp. minutes	180	
mouth alc. mark limit	500	
mouth alc. lower limit	30	
mouth alc. slope	6	
mouth alc. zero limit	50	
mouth alc. max. neg. sum	6	
mouth alc. max. 2nd derivative	35	

**ALCOTEST 9510 CERTIFICATION REPORT - WET ADJUST (PART I)**  
**South Brunswick**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0294  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Wet Adjust Record**

Wet Adjust File No.: 37 Wet Adjust Date: 01/15/2026 Wet Adjust No.: 2  
Wet Adjust Time: 07:30:41

Concentration: 0.100 %  
Adjusting Unit: X-Cal 2000 Adj. Unit Ser. No.: ARND-0002 Adj. Unit Exp.: 08/20/2026  
Solution Lot No.: 24210 Soln. Bottle No.: 757 Adjust Soln. Exp.: 06/11/2026

Preadjust Simulator Temp.: 34.00 degree C  
Postadjust Simulator Temp.: 34.01 degree C

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Fillimon - First Name: James MI: G Badge No.: 8306

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*For James Fillimon # 8306*

Signed:

Date: 01/15/2026

ID: 2673

**ALCOTEST 9510 CERTIFICATION REPORT - DRY ADJUST (PART II)**  
**South Brunswick**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0294  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Dry Adjust Record**

Dry Adjust File No.: 38 Dry Adjust Date: 01/15/2026 Dry Adjust No.: 2  
Dry Adjust Time: 07:48:42

Concentration: 0.100 %  
Dry Gas Lot No.: 302-403034216 Adjust Gas Exp.: 04/30/2027  
Barom. Model No.: Mensor CPG2300 Barom. Serial No.: 41001272 Barom. Cert. Exp.: 08/25/2026  
Pre-adjust Amb. Pressure: 999 hPa Post-adjust Amb. Pressure: 993 hPa

**Result**

**Procedure completed successfully.**

**Coordinator**

Last Name: Fillimon - First Name: James MI: G Badge No.: 8306

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*James Fillimon #8306*

Signed:

Date: 01/15/2026

ID: 2673

**ALCOTEST 9510 CERTIFICATION REPORT - LINEARITY (PART III)**  
**South Brunswick**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0294  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9

**Linearity Record**

Linearity File No.: 39 Lin. Date: 01/15/2026 Lin. No.: 2

0.040% Dry Gas Lot No.: 302-402730318 Adjust. Gas Exp.: 04/27/2026  
0.080% Dry Gas Lot No.: 302-402732434 Adjust. Gas Exp.: 04/28/2026  
0.160% Dry Gas Lot No.: 302-402922402 Adjust. Gas Exp.: 12/14/2026  
0.300% Dry Gas Lot No.: 302-402757700 Adjust. Gas Exp.: 05/26/2026

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	08:19:39		*TEST PASSED*
Control .04 Test 1 EC	0.040	08:20:17	994	*TEST PASSED*
Control .04 Test 1 IR	0.039	08:20:17	994	*TEST PASSED*
Ambient Air Blank	0.000	08:21:04		*TEST PASSED*
Control .04 Test 2 EC	0.040	08:21:19	994	*TEST PASSED*
Control .04 Test 2 IR	0.040	08:21:19	994	*TEST PASSED*
Ambient Air Blank	0.000	08:23:23		*TEST PASSED*
Control .08 Test 3 EC	0.079	08:24:00	994	*TEST PASSED*
Control .08 Test 3 IR	0.080	08:24:00	994	*TEST PASSED*
Ambient Air Blank	0.000	08:24:52		*TEST PASSED*
Control .08 Test 4 EC	0.080	08:25:06	994	*TEST PASSED*
Control .08 Test 4 IR	0.080	08:25:06	994	*TEST PASSED*
Ambient Air Blank	0.000	08:27:16		*TEST PASSED*
Control .16 Test 5 EC	0.156	08:27:51	994	*TEST PASSED*
Control .16 Test 5 IR	0.159	08:27:51	994	*TEST PASSED*
Ambient Air Blank	0.000	08:28:48		*TEST PASSED*
Control .16 Test 6 EC	0.158	08:29:00	994	*TEST PASSED*
Control .16 Test 6 IR	0.160	08:29:00	994	*TEST PASSED*
Ambient Air Blank	0.000	08:37:32		*TEST PASSED*
Control .30 Test 7 EC	0.297	08:38:07	994	*TEST PASSED*
Control .30 Test 7 IR	0.303	08:38:07	994	*TEST PASSED*
Ambient Air Blank	0.000	08:39:12		*TEST PASSED*
Control .30 Test 8 EC	0.300	08:39:24	994	*TEST PASSED*
Control .30 Test 8 IR	0.306	08:39:24	994	*TEST PASSED*
Ambient Air Blank	0.000	08:39:37		*TEST PASSED*

**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Fillimon - First Name: James MI: G Badge No.: 8306

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*Dr. James Fillimon # 8306*

Signed:

Date: 01/15/2026

ID: 2673

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 1**  
**South Brunswick**  
**SERIAL NUMBER: ARMJ-0294**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0294  
 Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
 Cyl1 Install File No.: 40 Cyl1 Install Date: 01/15/2026 Cyl1 Install No.: 2

**Control Tests (0.100%)**

Installation Inlet: #1 (Upper) Post test active Cyl.: #1 (Upper)  
 Dry Gas Lot No.: 302-403034219 Dry Gas Lot Exp.: 05/01/2027

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	08:52:07		*TEST PASSED*
Control Test 1			994	*TEST PASSED*
EC Result	0.099	08:52:52		*TEST PASSED*
IR Result	0.099	08:52:52		*TEST PASSED*
Ambient Air Blank	0.000	08:53:46		*TEST PASSED*
Control Test 2			994	*TEST PASSED*
EC Result	0.100	08:54:09		*TEST PASSED*
IR Result	0.100	08:54:09		*TEST PASSED*
Ambient Air Blank	0.000	08:55:04		*TEST PASSED*
Control Test 3			994	*TEST PASSED*
EC Result	0.100	08:55:28		*TEST PASSED*
IR Result	0.101	08:55:28		*TEST PASSED*
Ambient Air Blank	0.000	08:55:41		*TEST PASSED*

**Result**

**All tests within acceptable tolerance.**

**Coordinator**

Last Name: Fillimon - First Name: James MI: G Badge No.: 8306

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

*James Fillimon #8306*

Signed:

Date: 01/15/2026

ID: 2673

**ALCOTEST 9510 CYLINDER INSTALLATION REPORT - INLET 2**  
**South Brunswick**  
**SERIAL NUMBER: ARMJ-0294**

**Equipment**

Inst. Model No.: ALCOTEST 9510 Serial No.: ARMJ-0294  
Firmware: 8326739 1.5 Config.: 8326737 3.10 WinCE: 8326738 2.9  
Cyl2 Install File No.: 41 Cyl2 Install Date: 01/15/2026 Cyl2 Install No.: 2

**Control Tests (0.100%)**

Installation Inlet: #2 (Lower) Post test active Cyl.: #1 (Upper)  
Dry Gas Lot No.: 302-403368144 Dry Gas Lot Exp.: 06/13/2028

**Data Summary**

Function	Result %BAC	Time hh:mm:ss	Barometric Pres. [hPa]	Comment(s) or Status Code
Ambient Air Blank	0.000	09:03:01		*TEST PASSED*
Control Test 1			994	*TEST PASSED*
EC Result	0.099	09:03:46		*TEST PASSED*
IR Result	0.100	09:03:46		*TEST PASSED*
Ambient Air Blank	0.000	09:04:40		*TEST PASSED*
Control Test 2			994	*TEST PASSED*
EC Result	0.101	09:05:03		*TEST PASSED*
IR Result	0.101	09:05:03		*TEST PASSED*
Ambient Air Blank	0.000	09:05:57		*TEST PASSED*
Control Test 3			994	*TEST PASSED*
EC Result	0.101	09:06:21		*TEST PASSED*
IR Result	0.101	09:06:21		*TEST PASSED*
Ambient Air Blank	0.000	09:06:34		*TEST PASSED*


**Result**

All tests within acceptable tolerance.

**Coordinator**

Last Name: Fillimon - First Name: James MI: G Badge No.: 8306

On this date, I certified the above instrument in accordance with the Alcotest 9510 operator training and procedures established by the NJSP Office of Forensic Sciences.

 # 8306

Signed:

Date: 01/15/2026

ID: 2673

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036  
**DRAEGER MEDICAL SYSTEMS INC**

Sales order: 1130435101  
 Date: May 28, 2024

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
 ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
 CALGAZ LOT#: 302-403034219  
 ETHANOL IN NITROGEN

Manufactured Date: May 01, 2024  
 Product Expiration: May 01, 2027

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>	<b>PPM</b>	<b>( BrAC )</b>
ETHANOL	263.0	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

**Analytical:**


Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

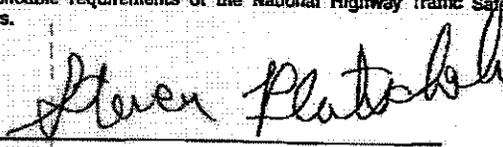APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
 821 Chesapeake Drive, Cambridge, MD 21613-0149  
 Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036  
**DRAEGER MEDICAL SYSTEMS INC**

Sales order: 1140199442  
 Date: June 18, 2025

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
 ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
 CALGAZ LOT#: 302-403368144  
 ETHANOL IN NITROGEN

Manufactured Date: June 13, 2025  
 Product Expiration: June 13, 2028

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>		
	PPM	( BrAC )
ETHANOL	262.7	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND49826	260.1

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44. Traceable certificate numbers 3445312 and 3398673.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.  
 Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.


\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
 CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

APPROVED BY: \_\_\_\_\_



"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
 821 Chesapeake Drive, Cambridge, MD 21613-0149  
 Phone: (410) 228-6400 Fax: (410) 228-4251

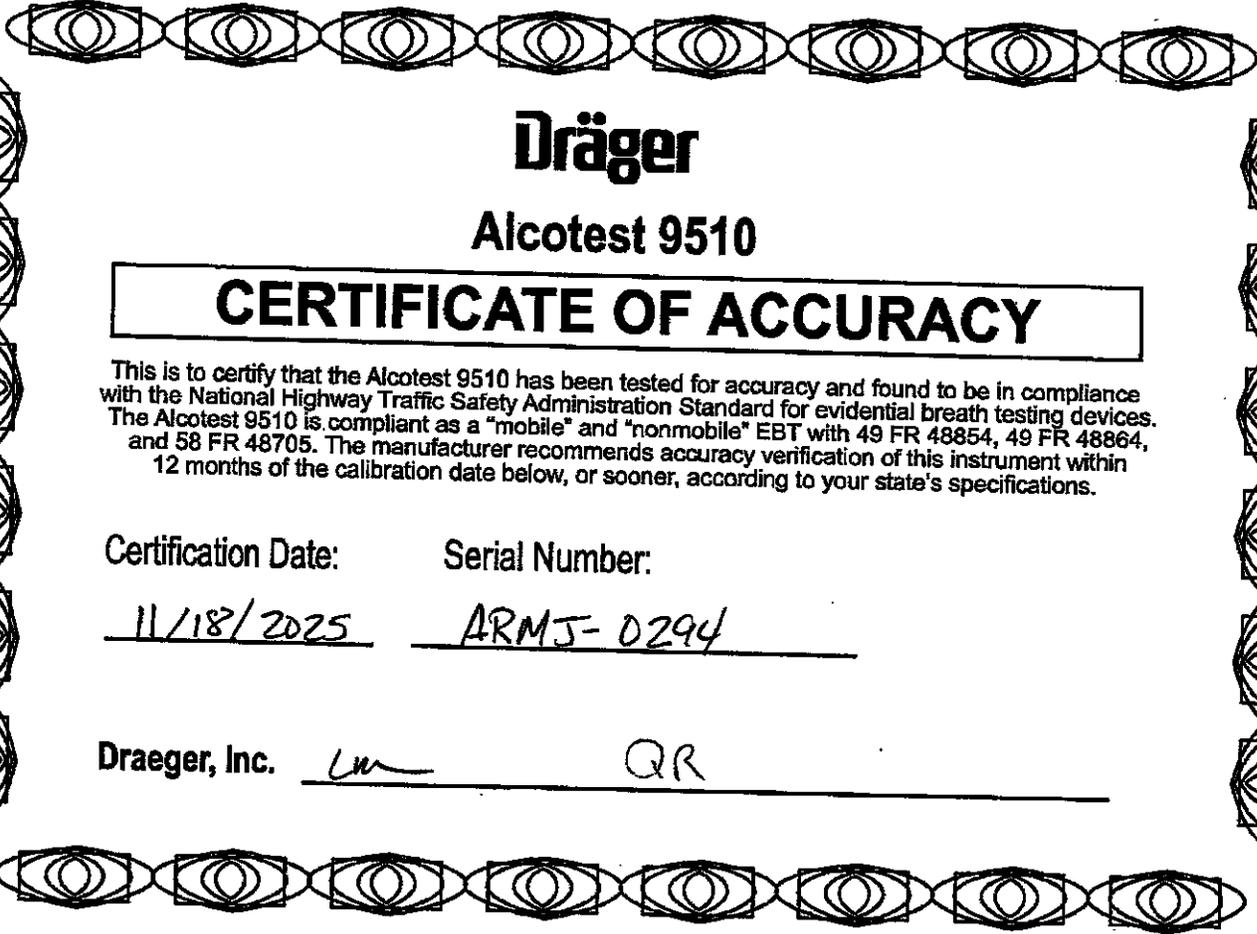

**Dräger**

**Alcotest 9510**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 9510 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest 9510 is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

11/18/2025

ARMJ-0294

Draeger, Inc.

LM

QR



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

TAHESHA L. WAY
Lt. Governor

MATTHEW J. PLATKIN
Attorney General

COLONEL PATRICK J. CALLAHAN
Superintendent

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 07/18/2024

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 24210

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1195 to 0.1217 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 11, 2026.

As OFS Director for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Michael Kennedy
Director
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 27 day of July, 2024.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



**CALIBRATED**  
BY TRANSCAT

# CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC.  
7286 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: SUC4303700862



Certificate/ISO Number: 5-F8B2G-280-1 Revision 0

Manufacturer: Draeger Safety AG & Co. KGaA  
Model Number: X-Cal 2000  
Description: Breath Alcohol Simulator  
Serial Number: ARND-0002  
ID: NONE

As-Found: Out Of Tolerance  
As-Left: In Tolerance

Issue Date: Aug 20, 2025  
Calibration Date: Aug 20, 2025  
Due Date: Aug 20, 2026

Calibrated To: Manufacturer Specification  
Calibration Procedure: 1-AC103619-2

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of this certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual DAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements, ISO 9001:2015, ANSI/NCSL 2546.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS 16949:2009, ISO/IEC 17025:2017, and ANSI/NCSL 2546.3-2006 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are appropriate to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio-type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.

Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-16. For mass calibrations, Conventional mass referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no./ID no. referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturer (OEM's) warranted specifications or the client's requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are depicted in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included in separate report(s).


**Notes:**

Unit was received Out of Tolerance and adjustments were made for best overall accuracy.

The OOT readings were verified.

# CALIBRATED BY TRANSCAT

# CERTIFICATE OF CALIBRATION

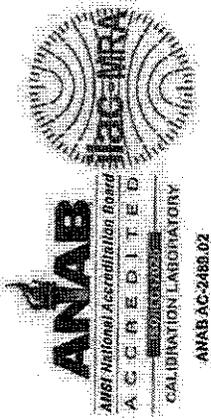

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: SUC4303700862

Certificate/SO Number: 5-F8B2G-280-1 Revision 0


### As Found Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Found	Cal Process		Units	TUR
						O	T		
<b>Function Checks</b>									
Bubble Check			P	P	P				
Seal Check			P	P	P				
<b>Temperature Source: Accuracy Test</b>									
Accuracy Test	34.00°C	±(0.02 °C)	33.88	34.02	33.97 °C	*	1.5e-002	1.6e-002	1.3:1
<b>Temperature Source: Stability Test</b>									
Stability Test	0.00°C	±(0.02 °C)	-0.02	0.02	0.00 °C		1.5e-002	1.6e-002	1.3:1

### As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Left	Cal Process		Units	TUR
						O	T		
<b>Function Checks</b>									
Bubble Check			P	P	P				
Seal Check			P	P	P				
<b>Temperature Source: Accuracy Test</b>									
Accuracy Test	34.00°C	±(0.02 °C)	33.88	34.02	34.00 °C		1.5e-002	1.6e-002	1.3:1
<b>Temperature Source: Stability Test</b>									
Stability Test	0.00°C	±(0.02 °C)	-0.02	0.02	0.00 °C		1.5e-002	1.6e-002	1.3:1

Field not applicable.

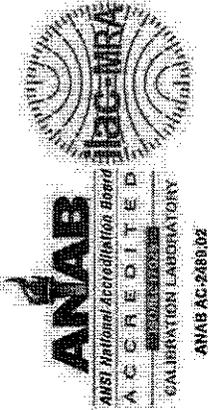

Customer: DRAEGER INC.  
7256 S. SAM HOUSTON PKWY W.  
STE. 100  
HOUSTON, TX. 77085  
PO Number: SUC4303700862

Certificate/SO Number: 5-F8B2G-280-1 Revision 0

### Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
05H1470	AccuMac Corporation	AM1760-12-S	Secondary SPRT	12-Aug-24	31-Aug-25	H32XM-4-1	AF/AL
HP927312	Hart Scientific/Fuke	1575	Super Thermometer	10-Jul-24	31-Jan-26	5-6HP027312-9-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

### Environmental Data

Temperature	Relative Humidity	Temp / RH Asset	Lab Area	Lab Description
69.70°F / 20.94°C	56.60%	DewK11	G	Temperature

### Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (quitters) is permitted after the "Determining and Verifying Out Of Tolerance (OOT), and/or Op Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.



Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: SUC4303700862

Certificate/ISO Number: 5-F8B2G-280-1 Revision 0

### Legend

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (K)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (#)
OOT	Out of Tolerance (*)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under test

**CALIBRATED**  
BY **TRANSCAT**

# CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
7266 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: SUC4303700862



Certificate/SO Number: 5-F8B2G-280-1 Revision 0

Calibrated At:  
16115 Park Row  
Houston, TX 77084

Facility Responsible:  
16115 Park Row  
Houston, TX 77084  
800-828-1470



Date Received: August 08, 2025  
Service Level: R9

Calibrated By:  
Electronically Signed By:  
Jose Martinez  
Calibration Technician


Aug 20, 2025  
11:56:02 -04:00

Reviewed By:  
Electronically Signed By:  
Luis Arap for  
Lab Manager

Aug 20, 2025  
13:57:50 -04:00

**CALIBRATED**  
BY **TRANSCAT**

# CERTIFICATE OF CALIBRATION

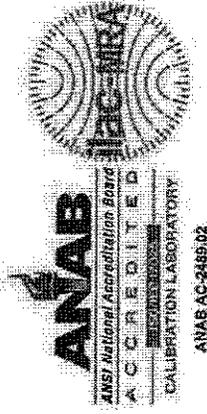

Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77065  
P.O Number: SUC4303700862

Certificate/ISO Number: 5-F8B2G-100-1 Revision 0

Manufacturer: Wika Instr/Mensor Corp/Trand  
Model Number: CPG2300  
Description: Portable Barometer  
Serial Number: 41001272  
ID: NONE

As-Found: Out Of Tolerance  
As-Left: In Tolerance  
Issue Date: Aug 25, 2025  
Calibration Date: Aug 25, 2025  
Due Date: Aug 25, 2026

Calibrated To: Manufacturer Specification  
Calibration Procedure: 1-AC107288-0

Transcat Calibration Laboratories have been audited and found in compliance with ISO/IEC 17025:2017. Accredited calibrations performed within the Lab Scope of Accreditation are indicated by the presence of the Accrediting Body Logo and Certificate Number. Any measurements on an accredited calibration not covered by the Lab Scope of Accreditation are listed in the notes section of the certificate. SCC, NRC, CLAS or ANAB do not guarantee the accuracy of an individual calibration by accredited laboratories.

Transcat calibrations, as applicable, are performed in compliance with the requirements of the Transcat Quality Manual QAC-P01-000, the customer Purchase Order and/or Quality Agreement requirements. ISO 9001:2015, ANSI/NCSL Z540.1-1994 (R2002), and ISO 10012:2003, as applicable. When specified contractually, the requirements of ISO TS 16949:2009, 10CFR21, 10CFR60, App. B, ASME NQA-1-2012, and ANSI/NCSL Z540.3-2005 (R2013) are also covered.

Complete records of work performed are maintained by Transcat and are available for inspection. Laboratory standards used in the performance of this calibration are listed on this certificate.

Transcat documents the traceability of measurements to the SI units through the National Institute of Standards and Technology (NIST), or the National Research Council of Canada (NRC), or other national measurement institutes (NMI) that are signatories to the CIPM Mutual Recognition Arrangement, or accepted fundamental and/or natural physical constants, or by the use of specified methods, consensus standards or ratio type measurements. Documentation supporting traceability information is available for review upon written request at a Transcat facility. The measured quantity and the measurement uncertainty are required for further dissemination of traceability.


Uncertainties are reported with a coverage factor  $k=2$ , providing a level of confidence of approximately 95%. All calibrations have been performed using processes having a TUR of 4:1 or better (3:1 for mass calibrations), unless otherwise noted. The Test Uncertainty Ratio (TUR) is calculated in accordance with NCSL International RP-18. For mass calibrations, Conventional mass, referenced to 8.0 g/cm<sup>3</sup>.

The results in this report relate only to the item calibrated or tested. Recorded calibration data is valid at the time of calibration within the stated uncertainties at the environmental conditions noted. The determination of compliance to the specification is specific to the model/serial no., referenced above based on the tolerances shown; these tolerances are either the original equipment manufacturers (OEM's) warranted specifications or the clients requested specifications. Any number of factors can cause a unit to drift out of tolerance at any time following its calibration. Limitations on the uses of this instrument are detailed in the OEM's operating instructions. This certificate may not be reproduced except in full, without the written approval of Transcat. Additional information, if applicable may be included on separate report(s).

**Notes:**

Received out of tolerance, Calibrated, Returned in tolerance. The COC readings were verified.


Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77065  
 PO Number: SUC4303709862

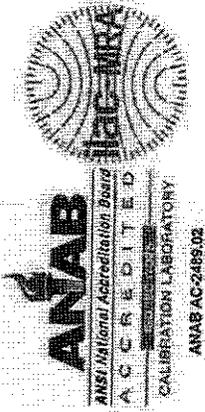

Certificate/ISO Number: 5-F8B2G-100-1 Revision 0

As Found Data

Description	Setpoints	Accuracy	Pressure Measure: 552 to 1172 mbara Range		High Limit	As Found	O	Cal Process	Measurement	Units	TUR
			Low Limit	Uncertainty (k=2; ±)							
	550.1 mbara	±(0.015% FS)	549.9	550.3	550.3	*	9.4e-003	6.1e-002	mbara	21.4 : 1	
	610.0 mbara	±(0.015% FS)	609.8	610.2	610.2	*	1.0e-002	5.9e-002	mbara	19.3 : 1	
	660.4 mbara	±(0.015% FS)	660.2	660.6	660.6	*	1.2e-002	5.9e-002	mbara	17.3 : 1	
	734.3 mbara	±(0.015% FS)	734.1	734.5	734.5	*	1.2e-002	5.9e-002	mbara	16.0 : 1	
	804.6 mbara	±(0.015% FS)	804.4	804.8	804.8	*	1.4e-002	6.0e-002	mbara	14.6 : 1	
	864.9 mbara	±(0.015% FS)	864.7	865.1	865.1	*	1.5e-002	6.0e-002	mbara	13.6 : 1	
	924.9 mbara	±(0.015% FS)	924.7	925.1	925.1	*	1.6e-002	6.0e-002	mbara	12.7 : 1	
	985.2 mbara	±(0.015% FS)	985.0	985.4	985.4	*	1.7e-002	6.0e-002	mbara	11.9 : 1	
	1043.9 mbara	±(0.015% FS)	1043.7	1044.1	1044.1	*	1.8e-002	6.1e-002	mbara	11.3 : 1	
	1114.2 mbara	±(0.015% FS)	1114.0	1114.4	1114.4	*	1.9e-002	6.1e-002	mbara	10.6 : 1	
	1174.5 mbara	±(0.015% FS)	1174.4	1174.8	1174.8	*	2.0e-002	6.1e-002	mbara	10.0 : 1	
	924.9 mbara	±(0.015% FS)	924.7	925.1	925.1	*	1.6e-002	6.0e-002	mbara	12.7 : 1	
	864.9 mbara	±(0.015% FS)	864.7	865.1	865.1	*	1.5e-002	6.0e-002	mbara	13.6 : 1	
	804.6 mbara	±(0.015% FS)	804.4	804.8	804.8	*	1.4e-002	6.0e-002	mbara	14.6 : 1	

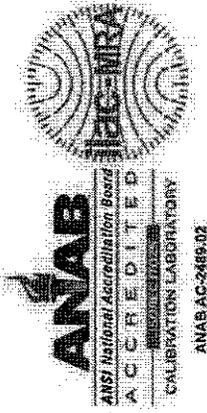

Customer: DRAEGER INC  
7266 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX 77085  
PO Number: SUC4303700862

Certificate/SO Number: 5-F8B2G-100-1 Revision 0

As Left Data

Description	Setpoints	Accuracy	Low Limit	High Limit	As Left	O		Cal Process Uncertainty (k=2; s)	Measurement Uncertainty (k=2; s)	Units	TUR
						Q	T				
Pressure Measure: 952 to 1172 mbara Range											
550.1mbara	±(0.015% FS)	649.9	550.3	550.1 mbara	550.1 mbara	9.4e-003	6.1e-002	mbara	21.4 : 1		
610.0mbara	±(0.015% FS)	609.8	610.2	610.0 mbara	610.0 mbara	1.0e-002	5.9e-002	mbara	19.3 : 1		
680.4mbara	±(0.015% FS)	680.2	680.6	680.4 mbara	680.4 mbara	1.2e-002	5.9e-002	mbara	17.3 : 1		
734.3mbara	±(0.015% FS)	734.1	734.5	734.3 mbara	734.3 mbara	1.2e-002	5.9e-002	mbara	16.0 : 1		
804.6mbara	±(0.015% FS)	804.4	804.8	804.7 mbara	804.7 mbara	1.4e-002	6.0e-002	mbara	14.6 : 1		
864.9mbara	±(0.015% FS)	864.7	865.1	865.0 mbara	865.0 mbara	1.5e-002	6.0e-002	mbara	13.6 : 1		
924.9mbara	±(0.015% FS)	924.7	925.1	925.0 mbara	925.0 mbara	1.6e-002	6.0e-002	mbara	12.7 : 1		
985.2mbara	±(0.015% FS)	985.0	985.4	985.3 mbara	985.3 mbara	1.7e-002	6.0e-002	mbara	11.9 : 1		
1043.8mbara	±(0.015% FS)	1043.6	1044.0	1043.8 mbara	1043.8 mbara	1.8e-002	6.1e-002	mbara	11.3 : 1		
1114.2mbara	±(0.015% FS)	1114.0	1114.4	1114.3 mbara	1114.3 mbara	1.9e-002	6.1e-002	mbara	10.6 : 1		
1174.6mbara	±(0.015% FS)	1174.4	1174.8	1174.6 mbara	1174.6 mbara	2.0e-002	6.1e-002	mbara	10.0 : 1		
924.9mbara	±(0.015% FS)	924.7	925.1	925.0 mbara	925.0 mbara	1.6e-002	6.0e-002	mbara	12.7 : 1		
864.9mbara	±(0.015% FS)	864.7	865.1	865.0 mbara	865.0 mbara	1.5e-002	6.0e-002	mbara	13.6 : 1		
804.6mbara	±(0.015% FS)	804.4	804.8	804.7 mbara	804.7 mbara	1.4e-002	6.0e-002	mbara	14.6 : 1		


Field not applicable.

Traceable Standards

Asset	Manufacturer	Model Number	Description	Cal Date	Due Date	Traceability Number	Use
DW11BA	Fluke/DH Instruments	PG7601	Piston Gauge	31-Jul-25	31-Jul-26	5-SDW11BA-20-1	AF/AL
DW11CA	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	5-Jun-25	30-Sep-25	5-SDW11CA-40-1	AF/AL
DW11LOW	Fluke/DH Instruments	PC-7100/7600-10-TC	Gas Piston-Cylinder Module	8-Apr-22	30-Apr-27	5-SDW11LOW-3-1	AF/AL
DW11MASS	Fluke/DH Instruments	MS-AMH-38	AMH Mass Set	5-Mar-25	31-Mar-26	5-SDW11MASS-12-1	AF/AL

The use of the standard is defined as: AF - used for as-found readings, AL - used for as-left readings.

Customer: DRAEGER INC.  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77065  
 PO Number: SUC4303700862

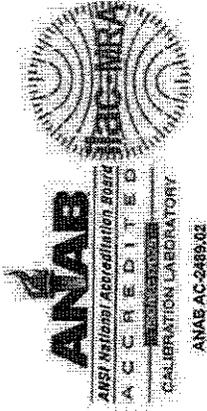

Certificate/SO Number: 5-F8B2G-100-1 Revision 0

### Environmental Data

	Temperature		Relative Humidity		Temp / RH Asset		Lab Area	Lab Description
	As Found:	As Left:	49.60%	52.20%	DewK10	DewK10		
	69.31°F / 20.73°C	69.27°F / 20.71°C					B	GP Pressure
							B	GP Pressure


### Decision Rule

When compliance statements are present, they are reported without factoring in the effects of uncertainty and comply with the guidelines as follows: The acceptance zone is defined as: less than or equal to the high limit, and/or greater than or equal to the low limit. The rejection zones are defined as greater than the high limit and/or less than the low limit. Single measurement results in the acceptance zone are identified as in-tolerance. Single measurement results in the rejection zone are identified as out-of-tolerance (OOT). When all measurement results are in the acceptance zone for repeated measurements, for the same characteristic, the test is identified as in-tolerance. For repeated characteristic measurements, a single measurement result in the rejection zone, will cause the test to be identified as out-of-tolerance (OOT). Data rejection for cause, (outliers) is permitted after the "Determining and Verifying Out Of Tolerance (OOT) and/or Op. Fail Readings" procedure outlined in this document has been completed and the anomalous reading cannot be repeated, and the anomalous reading does not represent the system under test. Statements of conformity are binary.

# CALIBRATED BY TRANSOIL

# CERTIFICATE OF CALIBRATION

Customer: DRAEGER INC  
 7256 S SAM HOUSTON PKWY W  
 STE 100  
 HOUSTON, TX 77085  
 PO Number: SUC4303700862

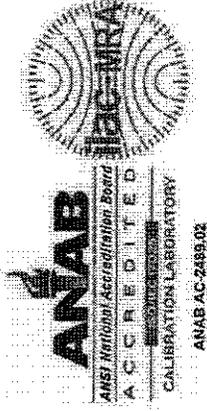

Certificate/SO Number: 5-F8B2G-100-1 Revision 0

## Legend

Topic	Description
Accuracy	UUT specification that establishes expected tolerances and a time limit (calibration interval) over which the instrument is expected to hold these tolerances
As Found	Initial measurement results
As Left	Measurement results after adjustment and/or repair
Blank Data Field	Test is not applicable for the UUT
Cal Process Uncertainty (CPU)	The uncertainty of calibration process for the reported measurement result
Calibration Date	Indicates the date that the calibration was completed
Cover Factor (k)	A measure of uncertainty that defines an interval about the measurement result
Due Date	Indicates the end of the calibration cycle as requested by the customer
Issue Date	Indicates the date that the calibration has passed the Data Review Process and was signed by an authorized signatory or the date that a revision to the original certificate has been issued
Low / High Limits	Establishes UUT acceptable performance limits for the test measurement
Measurement Uncertainty	The dispersion of the values attributed to a measured quantity
OOA	Out of Acceptance (%)
OOT	Out of Tolerance (%)
Setpoints	Measurement target values
Traceability	Unbroken chain of comparisons relating an instrument's measurements to a known standard(s)
Traceability Number	Unique identifier(s) used to document traceability of calibration standards
TUR	Test Uncertainty Ratio, ratio of the tolerance or specification of the test measurement in relation to the uncertainty in measurement results
UUT	Unit Under Test



**CALIBRATED**  
BY TRANSIT

# CERTIFICATE OF CALIBRATION



Customer: DRAEGER INC  
7256 S SAM HOUSTON PKWY W  
STE 100  
HOUSTON, TX, 77085  
PO Number: SUC4303700862

Certificate/SO Number: 5-F8B2G-100-1 Revision 0

Calibrated At: 10115 Park Row  
Houston, TX 77084  
Facility Responsible: 10115 Park Row  
Houston, TX 77084  
800-826-1470



Date Received: August 08, 2025  
Service Level: RG

**Calibrated By:**

Electronically Signed By:  
Evan Copeland

Evan Copeland  
Calibration Technician  
Aug 26, 2025  
13:31:47 -0400

**Reviewed By:**

Electronically Signed By:  
Graham Walker

Graham Walker  
Lab Manager  
Aug 26, 2025  
16:24:39 -0400

Certificate - Page 6 of 6  
Reprinted on August 27, 2025

Customer Number: 1-659111-000  
OPS-F20-014R11 07/27/23 FP001RS 4/8/2021

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401036

**DRAEGER MEDICAL SYSTEMS INC**

Sales order: 1130434779

Date: May 23, 2024

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-403034216

Manufactured Date: April 30, 2024

ETHANOL IN NITROGEN

Product Expiration: April 30, 2027

COMPONENT	PPM	( BrAC )
ETHANOL	260.5PPM	(0.100)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>		
	<b>PPM</b>	<b>( BrAC )</b>
ETHANOL	264.1	(0.101)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

**Analytical:**


Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

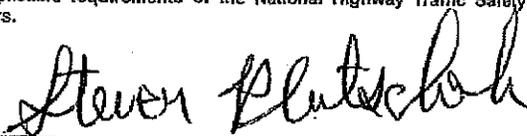APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
 821 Chesapeake Drive, Cambridge, MD 21613-0149  
 Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DEPT OF LAW AND PUBLIC SAFETY

Sales order: 1120656707  
Date: May 30, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater:  
CALGAZ LOT#: 302-402730318  
ETHANOL IN NITROGEN

Product Expiration: April 27, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	104.2PPM	(0.040)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	(BrAC)
ETHANOL	107.8	(0.041)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS:

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company, using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: April 27, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

CALGAZ, a division of Airgas USA LLC  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-6400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

DEPT OF LAW AND PUBLIC SAFETY

Sales order: 1120656618

Date: May 25, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402732434  
ETHANOL IN NITROGEN

Product Expiration: April 28, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	208.4PPM	(0.080)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	210.4	(0.081)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

### TRACEABILITY

#### Preparation:

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

#### Analytical:

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: April 28, 2023

APPROVED BY:

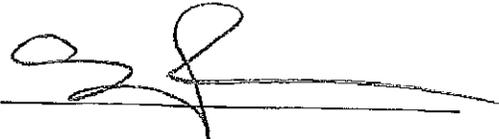

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**

821 Chesapeake Drive, Cambridge, MD 21613-0149

Phone: (410) 228-6400

Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Part Number: 4401040NJ  
DRAEGER MEDICAL SYSTEMS INC

Sales order: 1126209454  
Date: December 18, 2023

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer  
ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.  
CALGAZ LOT#: 302-402922402  
ETHANOL IN NITROGEN

Product Expiration: December 14, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	416.8PPM	(0.160)
NITROGEN	BAL	
AVERAGE ANALYTICAL VALUE	PPM	( BrAC )
ETHANOL	421.3	(0.162)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS  
TRACEABILITY  
Preparation:  
Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.  
Traceable certificate numbers 3445312 and 3398673.

Analytical:  
Analytical Instruments Calibrated Using NMI Traceable Standards.  
Certification Numbers: A679-20190918, D049803-20220329

No effecting environmental conditions during analysis.  
\*NMI is recognized by NIST through the Mutual Recognition Agreement (CIPM MRA).  
CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: December 14, 2023

APPROVED BY: 

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.85 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
821 Chesapeake Drive, Cambridge, MD 21613-0149  
Phone: (410) 228-8400 Fax: (410) 228-4251

# CERTIFICATE OF ANALYSIS

## EBS - ETHANOL BREATH STANDARD

Sales order: 120656632

Date: May 31, 2023

DEPT OF LAW AND PUBLIC SAFETY

METHOD OF ANALYSIS: IR Breath Alcohol Analyzer

ANALYTICAL ACCURACY: +/-0.002 BrAC or +/-2% whichever is greater.

CALGAZ LOT#: 302-402757700

ETHANOL IN NITROGEN

Product Expiration: May 26, 2026

COMPONENT	PPM	( BrAC )
ETHANOL	781.5PPM	(0.300)
NITROGEN	BAL	
<b>AVERAGE ANALYTICAL VALUE</b>		
ETHANOL	794.4	(0.305)

REFERENCE STANDARD	CYLINDER	CONCENTRATION PPM
N.M.I. TRACEABLE STANDARDS*	ND38424	260.7

\* CERTIFICATION TRACEABLE TO NATIONAL METROLOGY INSTITUTE TRACEABLE STANDARDS

**TRACEABILITY**

**Preparation:**

Gas mixtures manufactured with balances calibrated by an ISO 17025 accredited company using NIST traceable weights and meets or exceeds the requirements of NIST Handbook 44.

Traceable certificate numbers 3445312 and 3398673.

**Analytical:**

Analytical Instruments Calibrated Using NMI Traceable Standards.

Certification Numbers: A679-20190918, D049803-20220329


No effecting environmental conditions during analysis.

\*NMI is recognized by NIST through the Mutual Recognition Agreement (QRM MRA).

CALGAZ calibration devices were found to meet all applicable requirements of the National Highway Traffic Safety Administration Model Specifications for calibrating units for breath alcohol testers.

Manufactured Date: May 26, 2023

APPROVED BY: \_\_\_\_\_

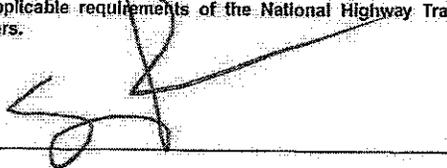

"We certify that all the cylinders for the Lot numbers identified herein are manufactured and tested within the requirements of CFR 49 part 178.65 and that physical and chemical test reports are on file and copies will be furnished upon request."

**CALGAZ, a division of Airgas USA LLC**  
 821 Chesapeake Drive, Cambridge, MD 21613-0149  
 Phone: (410) 228-6400 Fax: (410) 228-4251

DEPARTMENT OF  
**Traffic and Public Safety**  
*This is to certify that*

**James G. Fillimon**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF  
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 9510**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 3rd DAY OF October  
TWO THOUSAND AND Twenty Three

*[Signature]*  
COLONEL  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

DEPARTMENT OF  
**Traffic and Public Safety**  
*This is to certify that*

**James G. Fillimon**  
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF  
THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 9510**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 18th DAY OF November  
TWO THOUSAND AND Twenty Five

*[Signature]*  
COLONEL  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	4-10-25	MCPA	A.T.D.
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 2938 (Rev. 10/22)

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.			
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 2938 (Rev. 10/22)