

# Calibrating Unit New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0014
Location:	SOUTH BRUNSWICK POLICE		
Calibration File No.:	00714	Calib. Date:	06/28/2023
Certification File No.:	00715	Cert. No.:	00053
Linearity File No.:	00716	Cert. Date:	06/28/2023
Solution File No.:	00725	Lin. No.:	00042
Sequential File No.:	00725	Lin. Date:	06/28/2023
		Soln. No.:	00287
		Soln. Date:	09/25/2023
		File Date:	09/25/2023

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUF S3-0061
Control Solution %:	0.100%			Expires:	01/11/2025
Solution Control Lot:	23010			Bottle No.:	0732

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:07D		
Control 1 EC	0.100%	08:08D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:08D		
Control 2 EC	0.100%	08:09D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10D		
Control 3 EC	0.101%	08:10D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:10D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:11D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: GASSMAN

First Name: JASON

MI:

Signature: \_\_\_\_\_

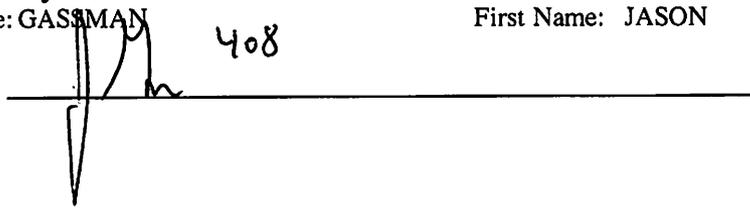

408

Badge No.: 408

Date: 09/25/2023